


BLOOD TRANSFUSION ARTEFACT RECORD	
NUMBER	AA-047
ITEM / TITLE	A BOOK OF (PINK) WHOLE HUMAN BLOOD GROUP B LABELS WITH SEQUENTIAL DONATION NUMBERS
PHYSICAL DESCRIPTION	A book of adhesive group B 'Whole Human Blood' group labels [number sequence B/58401 - B/58499 inclusive]. Each label page comprising six separate (by perforation) labels for labelling blood donations, samples and products (N.B.T.S. Sheffield 71).
OTHER INFORMATION	<p>Each numbered label page/set comprises six separate labels – each with the 'B/' number' information – for labelling different material, i.e.</p> <ol style="list-style-type: none"> <li>1. <i>Donation Label – includes spaces for entry of 'Rhesus Group', Taken on / at and Expiry date information as well as the following information:</i>  <i>Contents: Whole Blood 420cc – Acid Citrate Dextrose Anticoagulant</i>  <i>In Bottle: 120cc; In plastics Bag: 75cc</i>  <i>Test for Compatibility before use</i>  <i>Storage: Refrigerate at 4°C – 6°C (38° – 42°F)</i>  <i>The contents not to be used if visible signs of deterioration</i></li> <li>2. <i>Name and Initials – Dry Vial Sample Label</i></li> <li>3. <i>Processed Donation No. – Platelets – FFP – Cryo – GG</i></li> <li>4. <i>Name and initials</i></li> <li>5. <i>Name and Initials – Male/Female Low Hb Sample</i></li> <li>6. <i>'B/' number' information only</i></li> </ol> <p>Note: Adhesive on reverse of each page – many pages have adhered together over time.</p> <p>'N.B.T.S. Sheffield 71' indicates that the labels were used by the 'National Blood Transfusion Service, Sheffield Blood Centre' (England).</p>

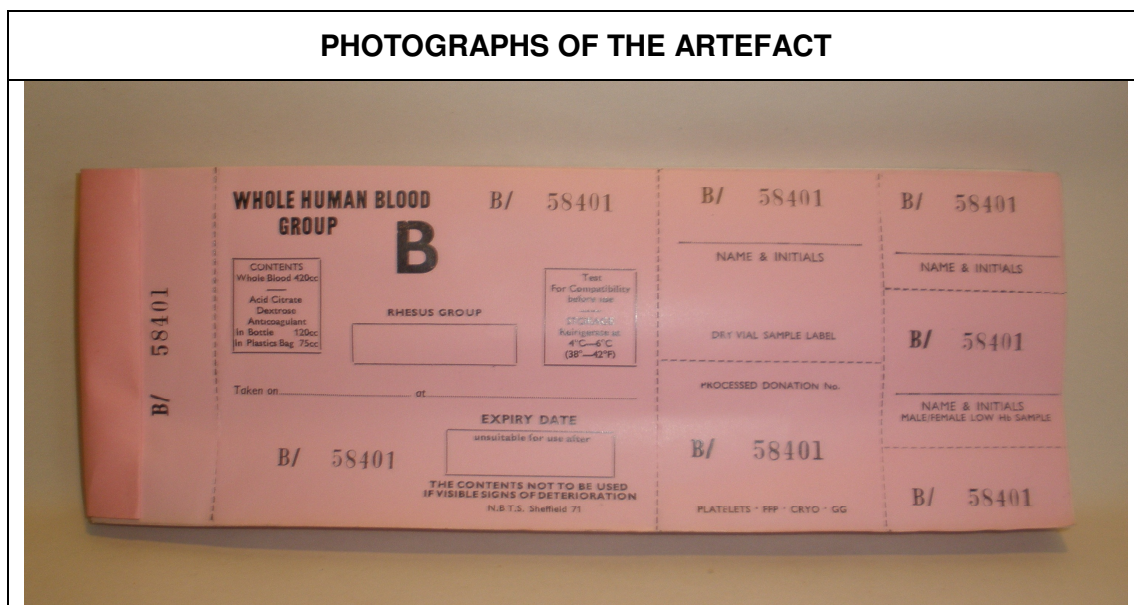

*Note: Additional photograph on the next page:*

WHOLE HUMAN BLOOD GROUP		B/ 58401	B/ 58401	B/ 58401
B/ 58401	<p><b>CONTENTS</b> Whole Blood 420cc</p> <p>Acid Citrate Dextrose Anticoagulant In Bottle 120cc In Plastic Bag 75cc</p>	<p><b>B</b></p> <p>RHESUS GROUP</p> <p>Test For Compatibility before use</p> <p>STORAGE Refrigerate at 4°C-6°C (38°-42°F)</p>	NAME & INITIALS	NAME & INITIALS
	<p>Taken on _____ at _____</p> <p>B/ 58401</p> <p>EXPIRY DATE</p> <p>unsuitable for use after</p> <p>THE CONTENTS NOT TO BE USED IF VISIBLE SIGNS OF DETERIORATION</p> <p>N.B.T.S. Sheffield 71</p>	<p>DRY VIAL SAMPLE LABEL</p> <p>PROCESSED DONATION No.</p> <p>B/ 58401</p> <p>PLATELETS - FFP - CRYO - GG</p>	<p>B/ 58401</p> <p>NAME &amp; INITIALS MALE/FEMALE LOW Hb SAMPLE</p> <p>B/ 58401</p>	